

CAUTION NOTICE

DVX001-CAU-2013

February 2013



HEAD OFFICE

Enterprise Drive
Westhill
Aberdeen
AB32 6TQ

T: +44 (0)1224 740145

F: +44 (0)1224 740172

Oral Nasal Caution Notice

DVX001-CAU-2013

Products Affected

SE351 Bell Survival Kit Pack 2


SE348 HRC Survival Kit

Following feedback from clients in the field we wish to make customers aware of changes to part numbers and components used within our range of Bell Survival Kit Lung Powered Scrubber Assemblies.

When conducting planned maintenance of these kits it may be necessary to replace the Oral Nasal Mask (SE455). If this is the case then please ensure that the corresponding Inlet & Exhaust Valves, spigots and blanking plugs are also replaced with the new versions.

GLOBAL LOCATIONS

Aberdeen
Chertsey
Bremen
Dubai
Cape Town
Perth
Sydney

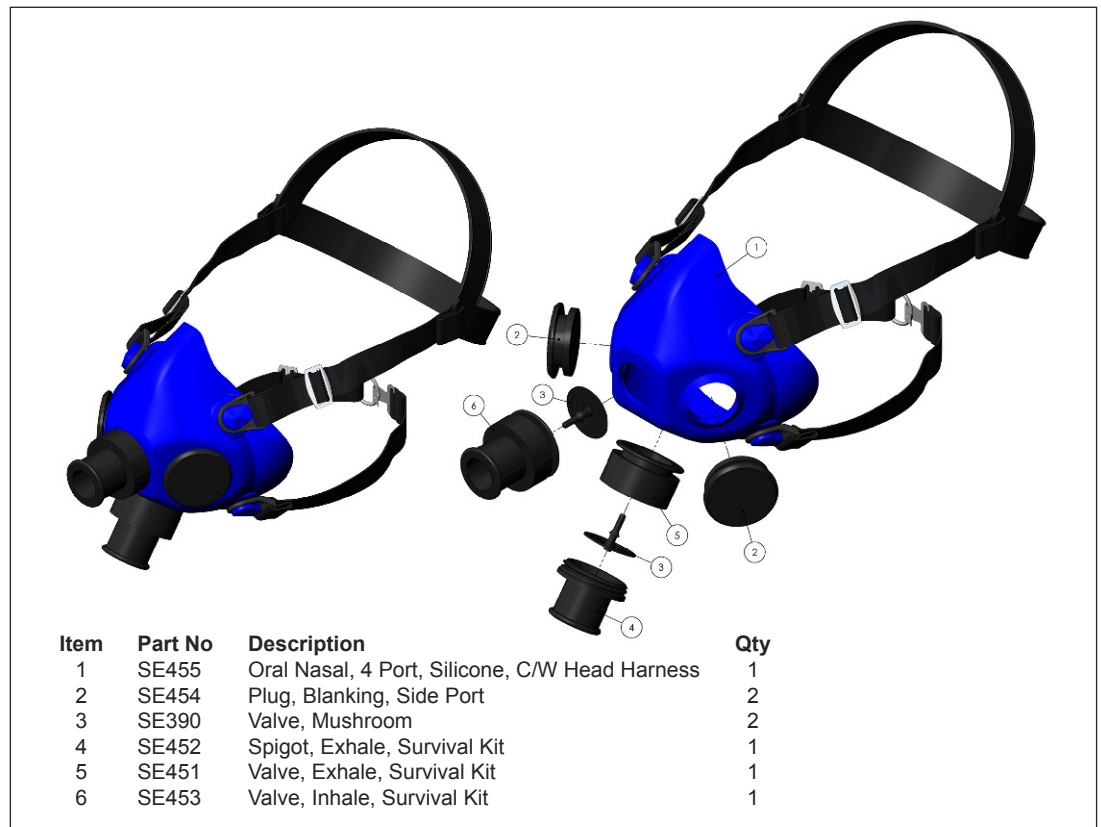

Item	Part No	Description	Qty
1	SE455	Oral Nasal, 4 Port, Silicone, C/W Head Harness	1
2	SE454	Plug, Blanking, Side Port	2
3	SE390	Valve, Mushroom	2
4	SE452	Spigot, Exhale, Survival Kit	1
5	SE451	Valve, Exhale, Survival Kit	1
6	SE453	Valve, Inhale, Survival Kit	1

THE VALVES, SPIGOTS AND PLUGS FROM THE PREVIOUS SURVIVAL KIT ARE NOT SIZED TO FIT THE NEW ORAL NASAL HENCE THE REQUIRED SEAL IS NOT ACHIEVED.

Signed:

Date: 5th February 2013

Kevin Smith General Manager - QHSE
for and on behalf of Divex Ltd.

Copyright 2013 Divex Limited. All Rights Reserved.

discover more
www.divexglobal.com

